

# Validation of the PHILIPS DL8760, oscillometric, upper arm blood pressure monitor, for self measurement in general population, according to the European Society of Hypertension International Protocol revision 2010

Mirna N. CHAHINE 1,2

Souad BOU HARB 1

Abd EL RAHMAN SAAD 1

Patrick SARKIS 1

Alaa AZAKI 1

Ali ALLOUCH 1

Aya HARB 1

Roland ASMAR 1,2

**Keywords:** PHILIPS® HBPM device; validation; Blood pressure measurement; ESH 2010 protocol

1 Faculty of Medical Sciences, Lebanese University, Hadath, Lebanon

2 Foundation-Medical Research Institutes (F-MRI®), Beirut, Lebanon.

Correspondence to PR ROLAND ASMAR, Foundation-Medical Research Institutes (F-MRI®), Hôpital Libanais-Geitaoui, 1st floor Achrafieh, Beirut, Lebanon.

Tel: +33640142239; e-mail: ra@cmcv.org

## Abstract

The PHILIPS DL8760, an upper arm blood pressure monitor, in oscillometry mode, for personal use, was validated, in a general population, according to the European Society of Hypertension International Protocol revision 2010. The protocol requirements were followed precisely. The device passed all of the requirements and, fulfilling the standards of the protocol, is recommended

## Device Details

Brand	PHILIPS
Model	DL8760
Manufacturer	PHILIPS COMPANY
Location	Upper Arm
Method	Oscillometry
Purpose	Self/ Home Measurement
Operation	Fully Automatic
Arm Cuff	Standard Adult: 22.0 cm to 42.0 cm



## Methodology

### Familiarisation

The validation team consisted of three persons: two observers trained in accurate BP measurement and a supervisor. The 2 observers have completed a training session. The agreement between the 2 observers was checked all over the evaluation period by the supervisor to make sure that the difference between the two is no more than 4 mmHg for systolic and diastolic BP values. Otherwise, the measurement should be repeated.

Two standard mercury sphygmomanometers, the components of which have been carefully checked before the study, were used by the 2 observers as a reference standard. Measurements were taken to the nearest 2 mmHg simultaneously by the 2 observers. Measurements made by the mercury sphygmomanometer were made on the left arm supported at heart level. Measurements made by the PHILIPS device were made on the same arm supported at the heart level as recommended

by the manufacturer. The circumference of the arm was measured to ensure that the cuff being used is adequate for the subject.

At all nine sequential same-arm measurements using the test instrument and the standard mercury sphygmomanometer were recorded as follows:

- BPA Entry BP, observers 1 and 2 each with the mercury standard
- BPB Device detection BP, supervisor
- BP1 Observers 1 and 2 with mercury standard
- BP2 Supervisor with the test instrument
- BP3 Observers 1 and 2 with mercury standard
- BP4 Supervisor with the test instrument
- BP5 Observers 1 and 2 with mercury standard
- BP6 Supervisor with the test instrument
- BP7 Observers 1 and 2 with mercury standard

#### Recruitment

Inclusion was carried out until 33 subjects at all, fulfilling the criteria of the international guidelines, have been included. The device was then evaluated according to the international protocol revised version 2010 requirements.

Recruitment of subjects was done in order to fulfill the recommended ranges of BP. There is three ranges for SBP and three for DBP:

	SBP (mmHg)	DBP (mmHg)
Low	90 – 129	40 – 79
Medium	130 – 160	80 – 100
High	161 - 180	101 - 130

For each subject, the device measurements BP2, BP4 and BP6 were first compared to observer measurements BP1, BP3 and BP5 respectively and then to observer measurements BP3, BP5 and BP7 respectively. Comparisons more favourable to the device were used. BP1, BP3, BP5 and BP7 were the means of the 2 observer measurements.

#### Screening and Recruitment Details


Screening and Recruitment		Recruitment Ranges			
			mmHg	All	On Rx
Total Screened	54				
Total Excluded	21				
Ranges Complete	0	Low	90 - 129	11	2
Ranges Adjustment	0	SBP Medium	130 - 160	10	5
Arrhythmias	0	High	161 - 180	10	10
Device Failure	0		> 180	2	
Poor Quality Sounds	1				
Cuff Size Unavailable	0	Low	< 40	0	2
Observer Disagreement	0		40 - 79	12	
Distribution	0	DBP Medium	80 - 100	11	6
Other Reasons	20	High	101 - 130	10	9
Total Recruited	33		> 130	0	

#### Procedure

The European Society of Hypertension International Protocol revision 2010 for the validation of blood pressure measuring devices in adults was followed precisely.[1] Overseen by an independent supervisor, measurements were recorded by two observers blinded from both each other's readings and from the device readings.



## Plots

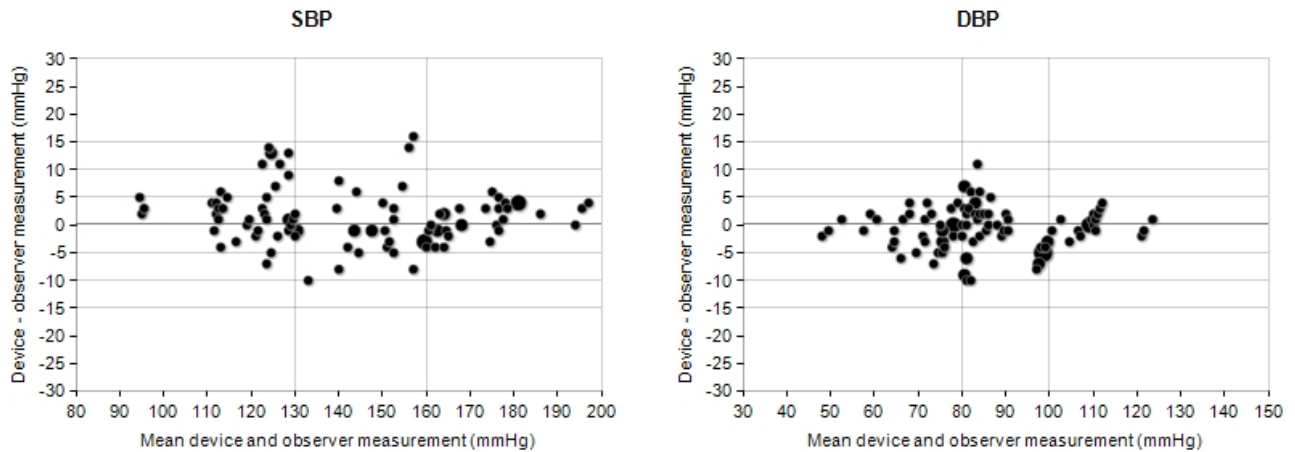

## Discussion

The objective of the study was to assess the accuracy of the PHILIPS device according to the international validation protocol revised version 2010 (1). The International Protocol has been published by the Working Group on Blood Pressure Monitoring of the European Society of Hypertension aiming to simplify the 2 main available guidelines, BHS and AAMI, without losing their merits.

We compared blood pressure values obtained by the cuff mercury sphygmomanometer at arm level with those obtained by the PHILIPS device. Mercury sphygmomanometer measurements are generally accepted as being the gold standard method of measuring blood pressure non-invasively.

This study showed the accuracy of the oscillometric device by fulfilling the International Protocol acquires. It should be emphasized, however, that each subject was in a correct seated position. For all measurements the arm was supported at the heart level. Recommendations given by the manufacturer are to achieve a correct posture before measuring blood pressure since an incorrect posture might give incorrect readings. The patient should relax and avoid wrist movements during measures like firm grips, large extensions or large flexions of the hand. It must, however, be emphasized that although the PHILIPS device designed for measuring blood pressure is accurate when tested according to the International Protocol.

This validation has been performed in general population; therefore the results cannot be extrapolated to other specific populations such as the elderly, pregnancy, obese, children or other populations.

## Conclusion

As the device has reached the required standards, it is recommended for personal use in a general population.

## References

1. O'Brien E, Atkins N, Stergiou G, Karpettas N, Parati G, Asmar R, Imai Y, Wang J, Mengden T, Shennan A; on behalf of the Working Group on Blood Pressure Monitoring of the European Society of Hypertension. European Society of Hypertension International Protocol revision 2010 for the Validation of Blood Pressure Measuring Devices In Adults. *Blood Press Monit* 2010;15:23–38.