

DECLARATION OF BLOOD PRESSURE MEASURING DEVICE EQUIVALENCE 2013

A SIGNED COPY WILL BE POSTED ON THE www.dableducational.org WEBSITE

SECTION A - Please complete all items.

I **Kevin Tan,** a Director of **Guangdong Transtek Medical Electronics Co.,Ltd**,
Name of a Company Director Company name

hereby state that there are no differences that will affect blood pressure measuring accuracy between the

Maker^a **Greater Goods, LLC.** Address **4427 Chouteau Ave. | St. Louis, MO 63110**
 Manufacturer^b **Transtek** Address **Zone A, No.105 ,Dongli Road, Torch Development District, Zhongshan,528437,Guangdong,China**
 Brand^c **Greater goods** Model^d **0040**

Blood pressure measuring device for which validation is claimed. If alternative model names are used, include all.

blood pressure measuring device and the validated blood pressure measuring device

Maker^a **Guangdong Transtek Medical Electronics Co.,Ltd** Address **Zone A, No.105 ,Dongli Road, Torch Development District, Zhongshan,528437,Guangdong,China**
 Manufacturer^b **Guangdong Transtek Medical Electronics Co.,Ltd** Address **Zone A, No.105 ,Dongli Road, Torch Development District, Zhongshan,528437,Guangdong,China**
 Brand^c **TRANSTEK** Model^d **TMB-1491**

Existing validated blood pressure measuring device.

which has previously passed the **2010** protocol, the results of which were published as follows:

Title: Validation of Transtek blood pressure monitor TMB-1491 for self-measurement according to the European Society of Hypertensio

Authors: Huiyong Tian, Sijian Zeng, Xiaoyan Zhong,Wei Gong and Wenju Liu

Full reference

The only differences between the devices involve the following components:

Tick one box for each item 1–18.

Part I	1	Algorithm for Oscillometric Measurements	Yes <input type="checkbox"/>	No <input checked="" type="checkbox"/>	N/A ^e <input type="checkbox"/>
	2	Algorithm for Auscultatory Measurements	Yes <input type="checkbox"/>	No <input type="checkbox"/>	N/A ^f <input checked="" type="checkbox"/>
	3	Artefact/Error Detection	Yes <input type="checkbox"/>	No <input checked="" type="checkbox"/>	
	4	Microphone(s)	Yes <input type="checkbox"/>	No <input type="checkbox"/>	N/A ^f <input checked="" type="checkbox"/>
	5	Pressure Transducer	Yes <input type="checkbox"/>	No <input checked="" type="checkbox"/>	
	6	Cuffs or Bladders	Yes <input type="checkbox"/>	No <input checked="" type="checkbox"/>	
	7	Inflation Mechanism	Yes <input type="checkbox"/>	No <input checked="" type="checkbox"/>	
	8	Deflation Mechanism	Yes <input type="checkbox"/>	No <input checked="" type="checkbox"/>	
Part II	9	Model Name or Number	Yes <input checked="" type="checkbox"/>	No <input type="checkbox"/>	
	10	Casing	Yes <input checked="" type="checkbox"/>	No <input type="checkbox"/>	
	11	Display	Yes <input type="checkbox"/>	No <input checked="" type="checkbox"/>	
	12	Carrying/Mounting Facilities	Yes <input checked="" type="checkbox"/>	No <input type="checkbox"/>	
	13	Software other than Algorithm	Yes <input type="checkbox"/>	No <input checked="" type="checkbox"/>	
	14	Memory Capacity/Number of stored measurements	Yes <input type="checkbox"/>	No <input checked="" type="checkbox"/>	
	15	Printing Facilities	Yes <input type="checkbox"/>	No <input type="checkbox"/>	N/A ^g <input checked="" type="checkbox"/>
	16	Communication Facilities	Yes <input type="checkbox"/>	No <input type="checkbox"/>	N/A ^g <input checked="" type="checkbox"/>
	17	Power Supply	Yes <input checked="" type="checkbox"/>	No <input type="checkbox"/>	
	18	Other Facilities	Yes <input type="checkbox"/>	No <input type="checkbox"/>	N/A ^g <input checked="" type="checkbox"/>

An explanation of each item ticked “Yes” must be included in Section B or on a separate sheet.

Notes: a Provide the name and address of the actual maker of the device.

b Provide the name and address of the legal manufacturer of the device, even if it is the same as that of the maker.

- c Provide the name of the brand under which it is sold, even if it is the same as that of the manufacturer or maker.
- d Provide the model name. If alternative or internal model names are used, include all. Each device must be uniquely identifiable.
- e Only tick N/A (Not Applicable) if neither device measures blood pressure using the oscillometric method.
- f Only tick N/A (Not Applicable) if neither device measures blood pressure using the auscultatory method.
- g Only tick N/A (Not Applicable) if neither device provides printing, communication or other facilities, as appropriate.

SECTION B An explanation for each item, 1 to 18, ticked "Yes" in Section A must be provided here or in an attached document. All differences between the devices must be described.

See attached document

SECTION C Please check that the following are included with the application

- A manual for the validated device
 - A manual for the device for which equivalence is being sought
 - An image of the validated device
 - An image of the device for which equivalence is being sought
 - An image of the screen layout of validated device*
 - An image of the screen layout of the device for which equivalence is being sought*
- * Screen layouts shown complete, and without obscuring labels or lines, in manuals need not be included separately.

SECTION D Complete all items, bar signatures and seal, online and print. Sign and seal it then send the original to our address below. Please email a signed copy of this form, together with the manuals and images for both devices, to info@dableducational.org.

Signature of Director Viya Qi Company Stamp/Seal

Name Kevin Tan

Date March 26, 2021

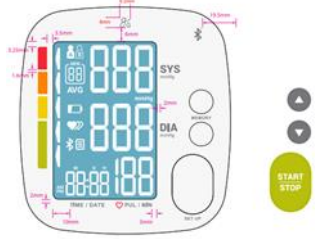

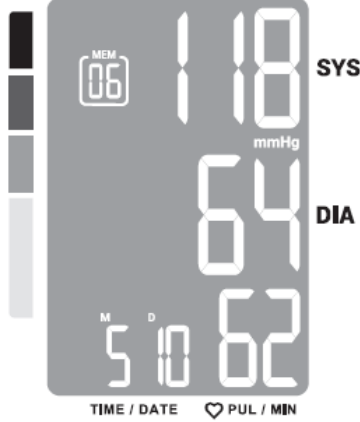
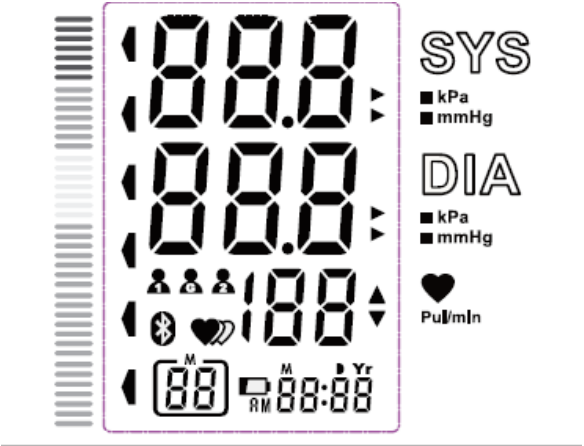
Signature of Witness Kevin Tan

Name Viya Qi

Address Zone A, No.105, Dongli Road, Torch Development District, Zhongshan, 528437, Guangdong, China



Comparison of the Greater Goods 0040 with the TRANSTEK TMB-1491

Devices – Item 9	Greater Goods 0040	TRANSTEK TMB-1491
Pictures	 <p>A photograph of the Greater Goods 0040 blood pressure monitor. It is a white, rectangular device with a blue LCD screen displaying '888' for systolic pressure, '888' for diastolic pressure, and '188' for pulse rate. The screen also shows 'SYS', 'DIA', and 'PUL' labels. There are two buttons on the right side and a 'START/STOP' button at the bottom.</p>	 <p>A photograph of the TRANSTEK TMB-1491 blood pressure monitor. It is a white, rectangular device with a blue LCD screen displaying '118' for systolic pressure, '64' for diastolic pressure, and '62' for pulse rate. The screen also shows 'SYS', 'DIA', and 'PUL' labels. There are two buttons on the right side and a 'START/STOP' button at the bottom.</p>
Display Image	 <p>A simulated display image for the Greater Goods 0040. The screen shows 'MEM 06' in the top left, '118' for SYS (mmHg), '64' for DIA (mmHg), and '5 10 62' for TIME / DATE and PUL / MIN. The screen also shows 'SYS', 'DIA', and 'PUL / MIN' labels.</p>	 <p>A simulated display image for the TRANSTEK TMB-1491. The screen shows '00.0' for SYS (kPa/mmHg), '00.0' for DIA (kPa/mmHg), and '188' for PUL (PUL/min). The screen also shows 'SYS', 'DIA', and 'PUL/min' labels, along with a heart icon and a pulse rate icon.</p>
Validation	Upper arm device for self measurement of blood pressure	ESH 2010
Category	Upper arm device for self measurement of blood pressure	Upper arm device for self measurement of blood pressure
Casing – Item 10	<p>Dimensions 140mm*130mm*55.6mm</p> <p>Ports Cuff port</p> <p>Features Cuff Trademark printing</p>	<p>Dimensions 110mm*100mm*41mm</p> <p>Ports Cuff port and DC power port</p> <p>Features Cuff and AC adaptor connectors Model name printing</p>

	Button printing	Button printing
Display – Item 11	LCD	LCD
Carrying/Mounting Facilities – Item 12	<i>Dimensions 195*140*90mm</i>	<i>Dimensions 182*130*80MM</i>
Software other than Algorithm – Item 13	<i>Dual Users 60 sets memories/per user AHA indicator mmHg unit mmHg unit</i>	<i>Dual Users 60 sets memories/per user WHO indicator mmHg unit</i>
Memory Capacity Item 14	<i>60 sets memories/per user</i>	<i>60 sets memories/per user</i>
Printing Facilities Item 15	N/A	N/A
Communication Facilities – Item 16	N/A	N/A
Power Supply Item 17	<i>6V DC 4×AAA batteries</i>	<i>6V DC Jack 4*AAA batteries</i>
Other differences	<i>Other Details on Equivalent device that are different to Validated device N/A</i>	<i>Other Details on Validated device that are different to Equivalent device N/A</i>
Same Criteria	<p>Measurement</p> <p><i>Accuracy Pressure within ±3mmHg(0.4kPa) Pulse value: ±5% Max</i></p> <p><i>Method Oscillographic testing mode</i></p> <p><i>Ranges SYS: 60mmHg~230mmHg (8.0kPa~30.7kPa) DIA: 40mmHg~130mmHg (5.3kPa~17.3kPa) Pulse value: (40-199)beat/minute</i></p> <p><i>Inflation Automatic inflation</i></p> <p><i>Deflation Automatic deflation</i></p>	<p>Measurement</p> <p><i>Accuracy Pressure: 5°C-40°C within ±3mmHg(0.4kPa) Pulse value: ±5%</i></p> <p><i>Method Oscillographic testing mode</i></p> <p><i>Ranges R SYS: 60mmHg~230mmHg (8.0kPa~30.7kPa) DIA: 40mmHg~130mmHg (5.3kPa~17.3kPa) Pulse value: (40-199) beat/minute</i></p> <p><i>Inflation Automatic inflation</i></p> <p><i>Deflation Automatic deflation</i></p>

	<p>Sensors PSG010S Measurements other than Blood Pressure Pulse rate</p> <p>Buttons/Switches Up/Down Delete Buttons Start/Stop & Select Button</p> <p>Display/Symbols/Indicators Preparation Automatic Zero setting</p> <p>Measurement Procedure Inflation symbol Pressure value indication Current time</p> <p>Measurement Records Systolic blood pressure (SYS) Diastolic blood pressure (DIA) Pulse rate Measurement time Memory Query symbol</p> <p>Power Low power</p> <p>Features Measuring during inflation</p> <p>Algorithms Equivalent device has the identical measurement algorithm as the validated device.</p>	<p>Sensors PSG010S Measurements other than Blood Pressure Pulse rate</p> <p>Buttons/Switches SYS button DIA button Start/Stop & Select Button</p> <p>Display/Symbols/Indicators Preparation Automatic Zero setting</p> <p>Measurement Procedure Inflation symbol Pressure value indication Current time</p> <p>Measurement Records Systolic blood pressure (SYS) Diastolic blood pressure (DIA) Pulse rate Measurement time Memory Query symbol</p> <p>Power Low power</p> <p>Features Measuring during inflation</p> <p>Algorithms Equivalent device has the identical measurement algorithm as the validated device.</p>
<p>Comparable Criteria</p>	<p>Measurement Cuffs (Please state sizes and materials used) About 22cm-42cm, large bore connector, Dacron material</p> <p>Measurement Records 60 sets/per user Display/Symbols/Indicators Post Measurement Systolic blood pressure (SYS)</p>	<p>Measurement Cuffs (Please state sizes and materials used) About 22cm or 32 or 22cm-42cm, polyester</p> <p>Measurement Records 60 sets/per user</p> <p>Display/Symbols/Indicators</p>

	<p><i>Diastolic blood pressure (DIA)</i> <i>Pulse rate</i> <i>Measurement time</i></p> <p>Function <i>Measure blood pressure and heart rate</i> <i>Recall measurement records</i> <i>Delete measurement records</i></p>	<p><i>Post Measurement</i> <i>Systolic blood pressure (SYS)</i> <i>Diastolic blood pressure (DIA)</i> <i>Pulse rate</i> <i>Measurement time</i></p> <p>Function <i>Measure blood pressure and heart rate</i> <i>Recall measurement records</i> <i>Delete measurement records</i></p>
--	---	--

Comments		
Recommendation	Recommended	
Date	April 2021	